

SAMPLE IDENTIFICATION

Peptide:	Retatrutide	Date Requested:	N/A
Client:	Integrity Peptides	Date Received:	May 29, 2026
Vendor:	Integrity Peptides	Date Tested:	Jun 5, 2026
Lot Number:	RT20-003	Date Reported:	Jun 8, 2026

HPLC-UV PURITY & CONTENT ANALYSIS

Expected Content 20.00 mg	Mass 22.48 mg	Purity 99.95%	Fill Accuracy 112.4%
-------------------------------------	-------------------------	-------------------------	--------------------------------


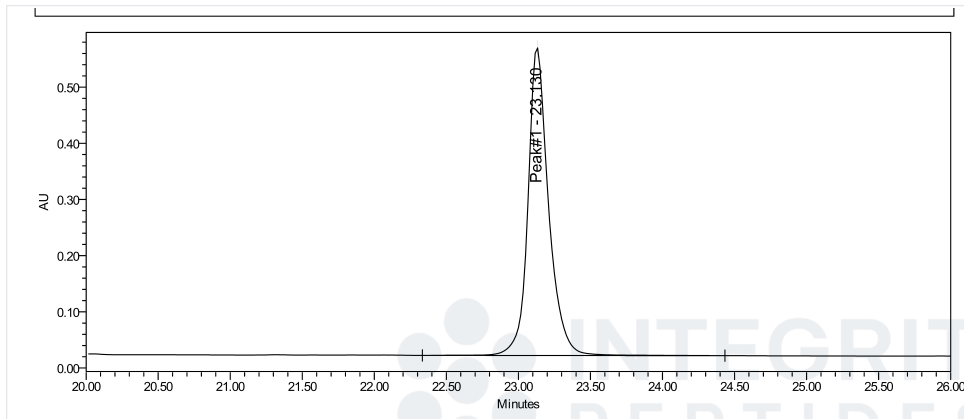


Fig. 1 - HPLC-UV Chromatogram at 214nm

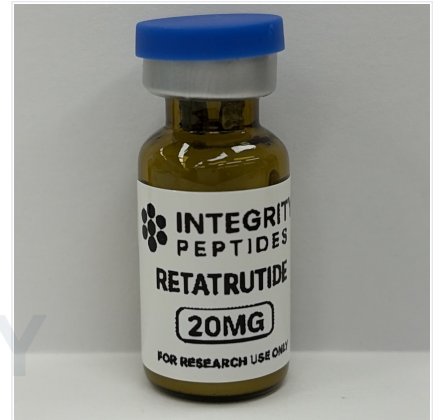

Appearance

Appearance:	White Lyophilized Powder
Cap Color:	Blue

BACTERIAL ENDOTOXIN TEST (USP <85>)

Method	Result	Specification	Verdict
Kinetic LAL (USP <85>)	< 0.125 EU/mL	<= 0.125 EU/mL	PASS

Interpretation: Endotoxin not detected (0.125 EU/mL) at validated 1:16 dilution (3.0 mL reconstituted vial).

This Certificate of Analysis is provided for informational and research purposes only.



Digital Verification